



Republic of the Philippines  
Department of Science and Technology



## PHILIPPINE NUCLEAR RESEARCH INSTITUTE

### INVITATION FOR NEGOTIATED PROCUREMENT

In view of the Two (2) Failed Public Bidding, the Philippine Nuclear Research Institute (PNRI) through its Bids and Awards Committee (BAC) invites PhilGEPS registered interested bidders to participate in the ***Negotiated Procurement for Supply of Labor, Tools, Materials and Technical Supervision for the Installation of Deionizer System*** with an Approved Budget for the Contract (ABC) of ***One Million Six Hundred Thousand Pesos (Php1,600,000.00)*** per BAC Resolution No. 030-2020 and in accordance with Section 53.1 of the 2016 Revised Implementing Rules and Regulations of Republic Act No. 9184, otherwise known as the "Government Procurement Act."

For more details on this project, please refer to Annex A (Technical Specifications) and Annex B (Drawing – Flow Diagram).

The following eligibility and technical documents as well as the Financial Proposal Form shall be submitted on March 18, 2021, Thursday, 10:00 AM at the 3<sup>rd</sup> Floor Conference Room, NART Building:

- (a) Valid PhilGEPS Certificate of Registration (Red or Platinum Membership) (all pages);
- (b) Request for Proposal (RFP) in compliance with the Technical Specifications (Annex A)

The Opening of Bids will be on March 18, 2021, 10:00 AM.

For further details, you may contact the BAC Secretariat at telephone nos. 920-87-60 or 929-60-11 to 19 loc. 259 (c/o Ricky C. Gabinete or Luzviminda B. Muyco) from 9:00 AM to 5:00 PM or visit our website at <http://www.pnri.dost.gov.ph>

The PNRI reserves the right to accept or reject any offer, to annul the negotiation process, and to reject all offers at any time prior to contract award, without hereby incurring any liability to affected suppliers.

**LUCILLE V. ABAD, Ph.D.**

Officer-In-Charge, ODD and Chairperson,  
Bids and Awards Committee

Address: Commonwealth Avenue, Diliman, Quezon City  
PO Box 213 UP Quezon City | PO Box 932 Manila | PO Box 1314 Central, Quezon City  
Telephone (632) 929-60-10 to 19 | Fax (632) 920-16-46

Technical Specifications

Item	Specification	Statement of Compliance
1.	<p><b>Supply of Labor, Tools, Materials and Technical Supervision for the Installation of Deionizer System</b></p> <p><b>Scope of Works:</b></p> <ol style="list-style-type: none"><li>1 hp pump-motor with built-in pressure switch</li><li>1" PVC schedule 80 pipes</li><li>Solenoid valves</li><li>PVC ball valves shall also be installed on the inlet and outlet pump</li><li>Pressure gage shall be installed on the outlet side of the pump</li><li>Control panel shall be located near the water tank</li><li>Circuit Breaker for Deionizer System</li><li>2 units of water in-line conductivity meter (for inlet and outlet)</li><li>1 unit of in-line ph meter(for outlet)</li><li>Mix bed ion exchange resin</li><li>Pre-filter</li><li>Required Water Conductivity: 0 to 1.5 micro Siemens per Centimeter (µS/cm)</li><li>Required Water ph: 4.5 to 7</li></ol> <p><b>Please see attached Diagram</b></p>	

***Company's Name:*** \_\_\_\_\_

***Duly authorized to sign Bid for and on behalf of:*** \_\_\_\_\_

***Date accomplished:*** \_\_\_\_\_



Diagrams for the Supply of Labor, Tools, Materials and Technical Supervision for the Installation of Deionizer System

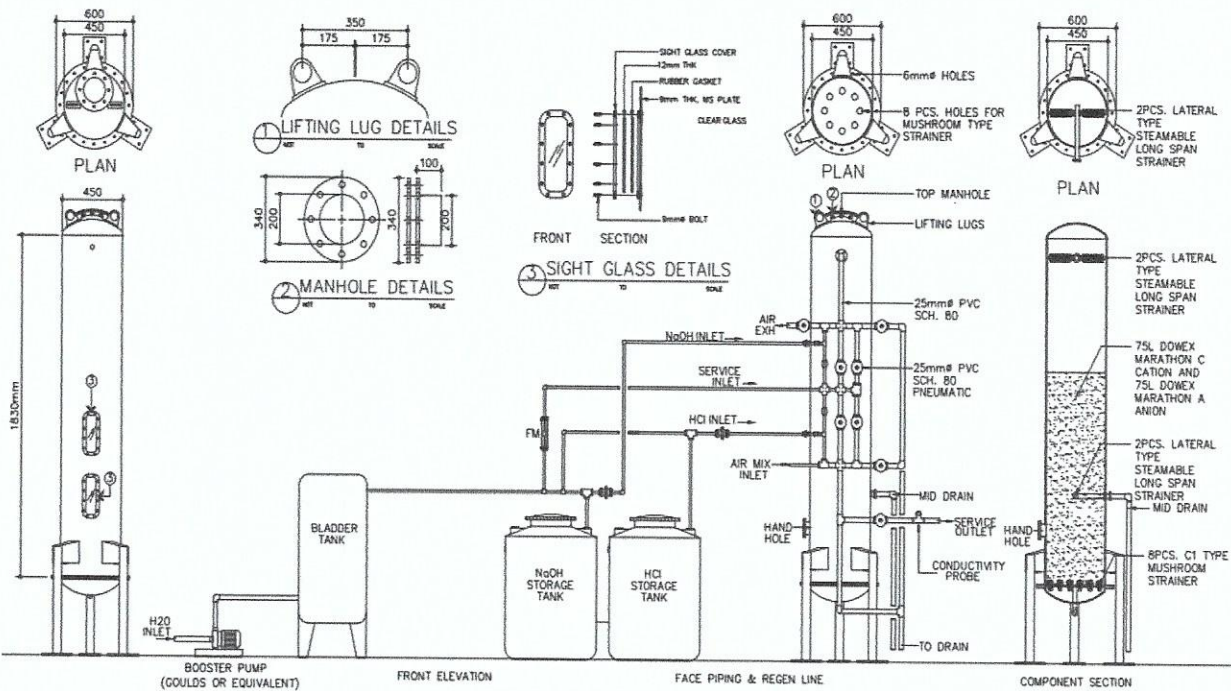


Figure: Sample flow diagram